Heathkit
CONDENSER CHECKER
MODEL C-2

The HEATH COMPANY
BENTON HARBOR, MICHIGAN

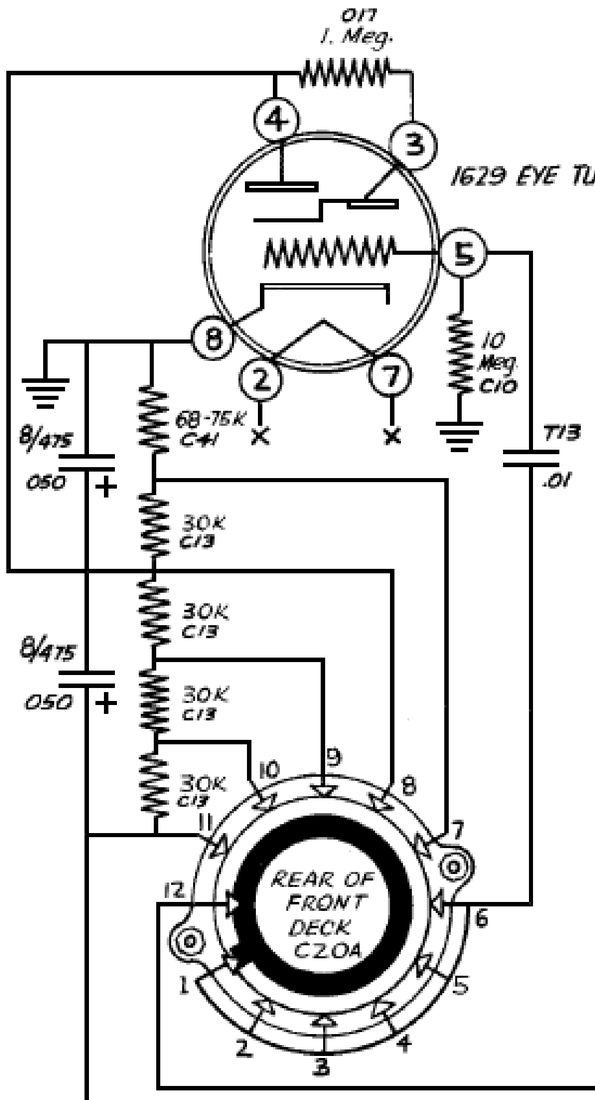

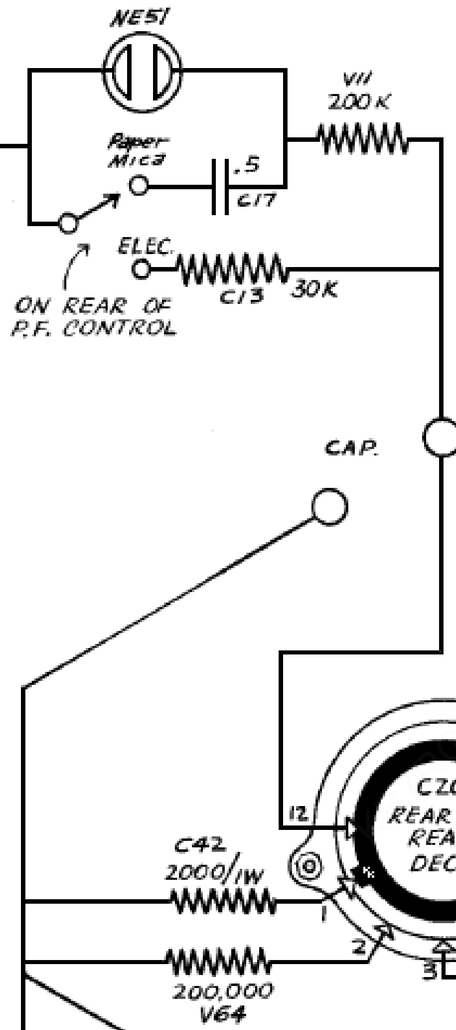

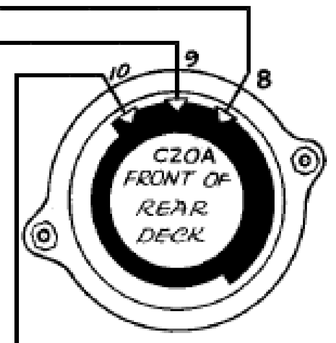

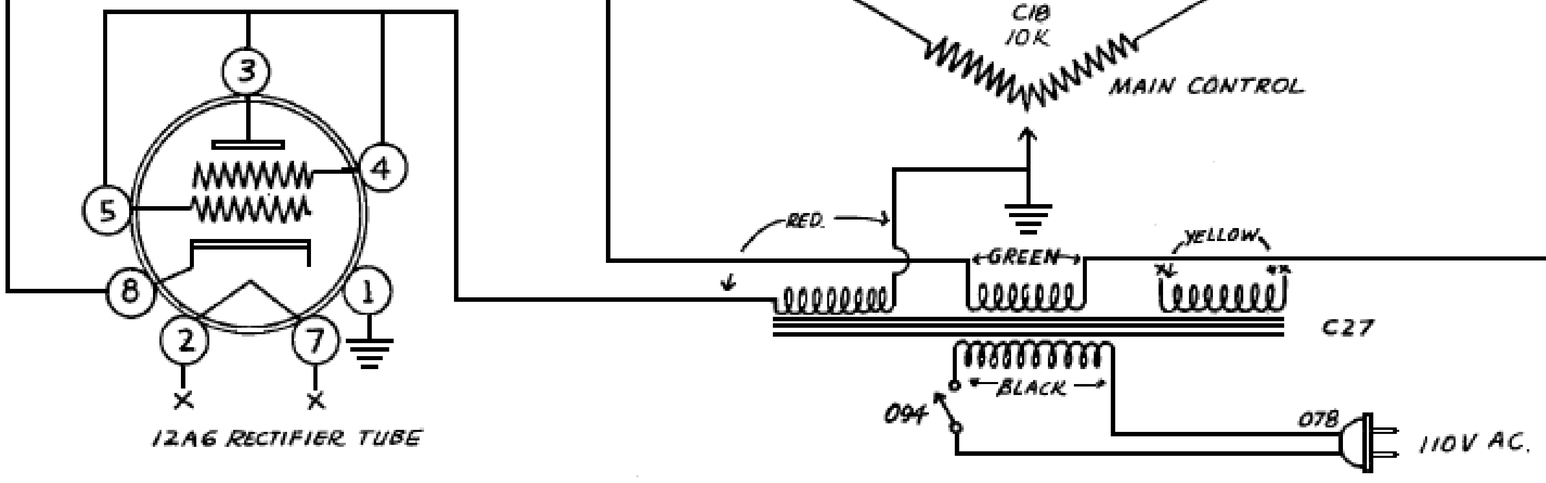

All Capacities in MFDS
Resistance in Ohms
k = 1000 Ohms
Meg. = 1,000,000 Ohms

Selector Switch shown looking from the rear in position "R"

1/15/50